Installation & Operation Manual

Quantim[®] QMC Series Mass Flow Controllers & Meters



Essential Instructions Read before proceeding!

Brooks Instrument designs, manufactures and tests its products to meet many national and international standards. These products must be properly installed, operated and maintained to ensure they continue to operate within their normal specifications. The following instructions must be adhered to and integrated into your safety program when installing, operating and maintaining Brooks Instrument products.

- · To ensure proper performance, use qualified personnel to install, operate, update, program and maintain the product.
- Read all instructions prior to installing, operating and servicing the product. If this instruction manual is not the correct manual, please see back cover for local sales office contact information. Save this instruction manual for future reference.

▲ WARNING: Do not operate this instrument in excess of the specifications listed in the Instruction and Operation Manual. Failure to heed this warning can result in serious personal injury and / or damage to the equipment.

- If you do not understand any of the instructions, contact your Brooks Instrument representative for clarification.
- Follow all warnings, cautions and instructions marked on and supplied with the product.

▲ WARNING: Prior to installation ensure this instrument has the required approval ratings to meet local and national codes. Failure to heed this warning can result in serious injury and / or damage to the equipment.

- Install your equipment as specified in the installation instructions of the appropriate instruction manual and per applicable local and national codes. Connect all products to the proper electrical and pressure sources.
- Operation: (1) Slowly initiate flow into the system. Open process valves slowly to avoid low surges. (2) Check for leaks around the flow meter inlet and outlet connections. If no leaks are present, bring the system up to the operating pressure.
- Please make sure that the process line pressure is removed prior to service. When replacement parts are required, ensure that qualified people use replacement parts specified by Brooks Instrument. Unauthorized parts and procedures can affect the product's performance and place the safe operation of your process at risk. Look-alike substitutions may result in fire, electrical hazards or improper operation.
- Ensure that all equipment doors are closed and protective covers are in place to prevent electrical shock and personal injury, except when maintenance is being performed by qualified persons.

▲ WARNING: For liquid flow devices, if the inlet and outlet valves adjacent to the devices are to be closed for any reason, the devices must be completely drained. Failure to do so may result in thermal expansion of the liquid that can rupture the device and may cause personal injury.

European Pressure Equipment Directive (PED)

All pressure equipment with an internal pressure gauge greater than 0.5 bar (g) and a size larger than 25mm or 1" (inch) falls under the Pressure Equipment Directive (PED).

- The Specifications Section of this manual contains instructions related to the PED directive.
- Products described in this manual are in compliance with EN directive 2014/34/EU.
- All Brooks Instrument Flowmeters fall under fluid group 1.
- Products larger than 25mm or 1" (inch) are in compliance with EN directive 2014/34/EU.
- Products of 25mm or 1" (inch) or smaller are Sound Engineering Practice (SEP).

European Electromagnetic Compatibility (EMC)

The Brooks Instrument (electric/electronic) equipment bearing the CE mark has been successfully tested to the regulations of the Electro Magnetic Compatibility (EMC directive 2014/30/EU).

Special attention however is required when selecting the signal cable to be used with CE marked equipment.

Quality of the signal cable, cable glands and connectors:

Brooks Instrument supplies a limited selection of high quality cable(s) which meets the specifications for CE certification.

If you provide your own signal cable you should use a cable which is overall completely screened with a 100% shield.

"D" or "Circular" type connectors used should be shielded with a metal shield. If applicable, metal cable glands must be used providing cable screens clamping. The cable screen should be connected to the metal shell or gland and shielded at both ends over 360 Degrees.

The shield should be terminated to an earth ground. Card Edge Connectors are standard non-metallic. The cables used must be screened with 100% shield to comply with CE certification. The shield should be terminated to an earth ground. For additional instruction regarding Protective Earth (PE) Connections please refer to Section 2, **Electrical Interface** page 29.

For pin configuration: Please refer to the enclosed Instruction Manual.

ESD (Electrostatic Discharge)

▲ CAUTION: This instrument contains electronic components that are susceptible to damage by static electricity. Proper handling procedures must be observed during the removal, installation or other handling of internal circuit boards or devices.

Handling Procedure:

- 1. Power to unit must be removed.
- 2. Personnel must be grounded, via a wrist strap or other safe, suitable means before any printed circuit card or other internal device is installed, removed or adjusted.
- Printed circuit boards must be transported in a conductive container. Boards must not be removed from protective enclosure until immediately before installation. Removed boards must immediately be placed in protective container for transport, storage or return to factory.

Comments

This instrument is not unique in its content of ESD (electrostatic discharge) sensitive components. Most modern electronic designs contain components that utilize metal oxide technology (NMOS, SMOS, etc.) Experience has proven that even small amonts of static electricity can damage or destroy these devices. Damaged components, even though they appear to function properly, exhibit early failure.

Brooks Instrument Quick Start Guide


Step 1: Location/Orientation


The instrument may be located anywhere in the process line, as long as the following conditions are met:


- Before operation, you must be able to stop flow through the meter. During the zeroing procedure, flow must be stopped completely, and the flow meter sensor tube must be full of process fluid to achieve an accurate zero.
- During operation, the flow sensor tube must be full of process fluid.
- Ambient temperature must remain between 0° and 60°C (32°F and 140°F).
- The instrument (cable connections, wiring compartments and/or conduit openings) should be accessible for service.

ACAUTION


When installing the Mass Flow device, care should be taken to prevent foreign materials from entering the instrument's inlet or outlet. Internal passages are very small. It is recommended that an inlet filter be used to limit the chance of clogging. Do not remove the protective end-caps until the actual moment of installation. When used with reactive fluids (some of which may be toxic or moisture sensitive), contamination or corrosion may occur as a result of plumbing leaks or improper purging. Plumbing should be checked carefully for leaks. Care must be taken to thoroughly purge / dry down the system before introduction of any moisture sensitive process fluid.

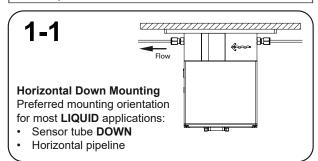


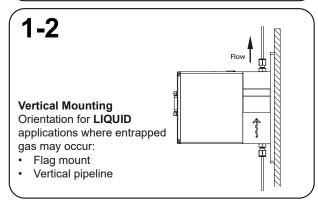

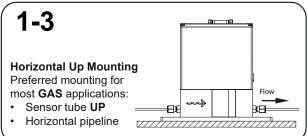

Step 2: Mounting the Quantim

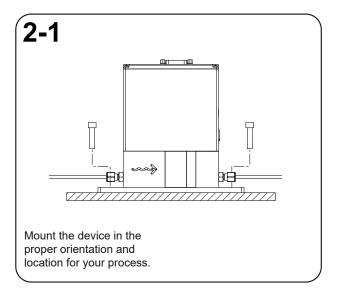

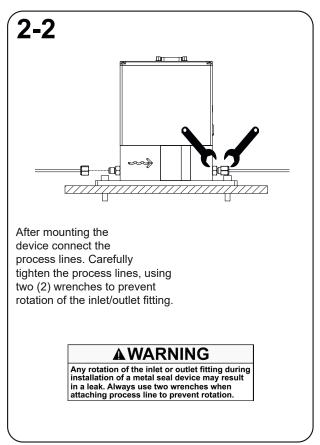


Brooks Instrument Quick Start Guide


Step 3A: Electrical Connections IP40 Meter/Controller

D-Connector Functions Legends:
• = Feature Available


N/A = Not Available


NOTE: Chassis ground is available through the D-Connector back shell.

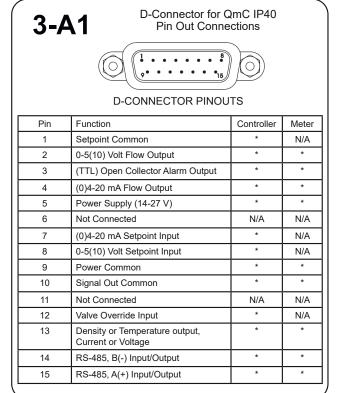

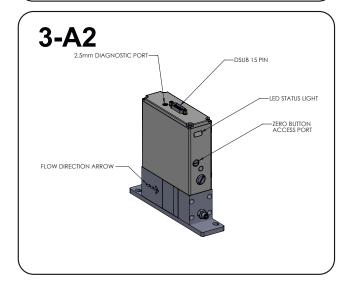

Step 3B: Electrical Connections Meter/Controller IP66 or Class 1 Division 2 / Zone 2

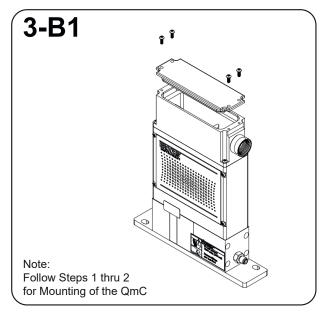

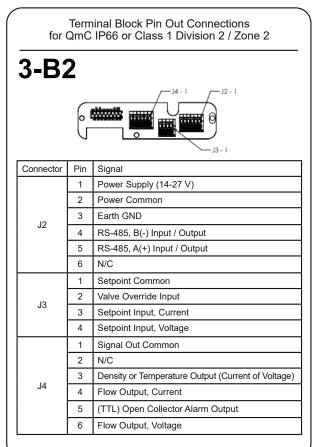

Brooks Instrument Quick Start Guide

Step 4: Zeroing Procedure

To assure measurement accuracy, the instrument must be zeroed to the operational installation conditions:

- Apply power to instrument for approximately 45 minutes to reach a stable thermal condition prior to applying flow.
- Flow the process fluid into the instrument and allow sufficient time for the sensor to reach normal operating temperature.
- · Close the shutoff valve downstream to eliminate any pressure differential across the instrument.
- After confirming a NO flow condition, press the zeroing button for at least 3 seconds
- · Zeroing button is located on the side of the instrument's housing
- The zeroing process takes approximately 60 seconds. Status light will flash red.
- · A solid Green LED means a successful zero.
- · A solid Red LED means an unsuccessful zero.

Note: If solid Red LED is indicated, recycle power and repeat zeroing procedure or contact Technical Services at Brooks Instrument

Step 5: Operation

After the flowmeter or flow controller has been installed in the system it is ready for operation.

Meter: The meter will provide a flow signal proportional to the full scale flow of the device as indicated on the device label. Controller: You must provide a setpoint/command signal to the controller. The controller will read the setpoint signal and will automatically adjust the valve to the appropriate position to achieve the desired flow and will provide a flow signal proportional to the full scale flow of the device as indicated on the device label.

Equipment Receipt and Return Procedures

Receipt of Equipment

When the equipment is received, the outside packing case should be checked for damage incurred during shipment. If the packing case is damaged, the local carrier should be notified at once regarding his liability. A report should be submitted to the nearest Brooks Instrument location listed on the Global Service Network page on our website: brooksinstrument.com/service-support Remove the envelope containing the packing list. Carefully remove the instrument from the packing case. Make sure spare parts are not discarded with the packing materials. Inspect for damaged or missing parts.

Return Shipment

Prior to returning any instrument to the factory for any reason, visit our website for instructions on how to obtain a Return Materials Authorization Number (RMA#) and complete a Decontamination Statement to accompany it: brooksinstrument.com/service-support All instruments returned to Brooks also require a Material Safety Data Sheet (MSDS) for the fluid(s) used in the instrument. Failure to provide this information will delay processing of the instrument. Instrument must have been purged in accordance with the following:

▲ WARNING

Before returning the device, purge thoroughly with a dry inert gas such as Nitrogen before disconnecting process connections. Failure to correctly purge the instrument could result in fire, explosion or death. Corrosion or contamination may occur upon exposure to air.

▲WARNING

- Read all instructions prior to installing, operating and servicing this product.
- Follow all warnings, cautions and instructions marked on and supplied with this product.
- Install your equipment as specified in the installation instructions in the appropriate instruction manual and per local and national codes. Connect all products to the proper electrical and pressure sources.
- Ensure that all equipment doors are closed and protective covers are in place, except when maintenance is being performed by qualified persons, to prevent electrical shock and personal injury.
- Do not operate this instrument in excess of the specifications marked on and supplied with this product. Failure to heed this warning can result in serious personal injury and/or damage to the equipment.
- Before operating the device, ensure all electrical connections have been properly terminated.
- If it becomes necessary to remove the device from the system, power to the device must be disconnected.
- If it becomes necessary to remove the device from the system after exposure to toxic, pyrophoric, flammable or corrosive gas, purge the device thoroughly with a dry inert gas such as nitrogen before disconnecting the gas connections. Failure to correctly purge the device could result in fire, explosion or death. Corrosion or contamination of the device upon exposure to air may also occur.

A CAUTION

- Incorrect voltage will cause flowmeter damage or failure.
- QUANTIM is an input sinking device. Do not use a current sinking PLC output card.
- QUANTIM sources its own 4-20mA output signal. Do not source this output with an external supply.

Global Headquarters

Brooks Instrument 407 West Vine Street Hatfield, PA 19440-0903 USA Toll-Free (USA): 888-554-FLOW Tel (215) 362 3700 Fax (215) 362 3745 BrooksAm@BrooksInstrument.com

A list of all Brooks Instrument locations and contact details can be found at www.BrooksInstrument.com

Brooks and Quantim are trademarks of Brooks Instrument, LLC. All other trademarks are property of their respective owners.

P/N: 541B236AAG/A Reference: 834z986





A list of all Brooks Instrument locations and contact details can be found at www.BrooksInstrument.com

©Copyright 2025 Brooks Instrument, LLC All rights reserved. Printed in U.S.A.

INSTRUMENT

Beyond Measure

Brooks Instrument Contents

Quick Start Instructions

Quick Start Instructions Location / Orientation and Mounting	QS-1
Quick Start Instructions Electrical Connections	QS-2
Quick Start Instructions Zeroing Procedure and Operations	QS-3
Quick Start Instructions Equipment Receipt and Return	QS-3
Quick Start Instructions Warning and Caution	QS-3
Section 1 Introduction	
How to Use This Manual	1
Description	
Performance Specifications	
Dimensions	
Section 2 Installation	
General	
Receipt of Equipment	
Recommended Storage PracticeReturn Shipment	
Transit Precautions	
Fluid Connections	
Mechanical Installation	
Process Mounting	
Electrical Interfacing	
Interconnection with Peripheral Equipment	
Section 3 Operation	
Operating Procedure	
Zero Adjustment	
Calibration Procedure	20
Section 4 Maintenance & Troubleshooting	
General	
Maintenance & Troubleshooting	
Warranty, Local Sales/Service Contact Information	
Warranty Local Sales/Service Contact Information	Back Cove

Brooks Instrument Contents

Figures

	1-1 Dimensional Drawing QMC IP40.	
	1-2 Dimensional Drawing QMC IP6x / Class 1 Division 2 Zone 2	
	1-3 Dimensional Drawing QMC Bottom View	
	1-4 Lay-In Dimensions Integral Valve	
	1-5 D-Connector Electrical Pin Connections	
	1-6 Terminal Block Pinout Connections for IP66 of Class T Division 27 Zone 2)
	2-1 Flow Direction Through the Quantim, as Indicated by the Arrow	
	Engraved on the Meter/Controller Body1	0
	2-2 Horizontal Inverted Installation	
	2-3 Horizontal Right Side Up Installation1	1
	2-4 Vertical Flow Up Installation	
	2-5 Alarm Output Wiring Options1	
	2-6 General Wiring1	
	2-7 Wire Color Codes for 'D' Connector Assembly	7
	3-1 Location of the LEDs, Zero Button and Diagnostic Port, IP40 Device	8
	3-2 Location of the LEDs, Zero Button and Diagnostic Port, IP6x Device	3
	4-1 Bench Troubleshooting Circuit	ô
Tables		
	1-1 Product Specifications	2
	2-1 Electrical Interfacing for Quantim QMC IP40	3
	2-2 Electrical Interfacing for Quantim QMC IP6x	
	4-1 Maintenance & Troubleshooting	3

How to Use This Manual

It is recommended to read this manual before installing, operating or troubleshooting your Quantim® QMC Series Mass Flow Meter or Controller.

This manual is organized into the following sections:

Section 1. Introduction
Section 2. Installation
Section 3. Operation

Section 4. Maintenance & Troubleshooting

Back Cover Warranty, Local Sales/Service Contact Information

The Quality System at Brooks Instrument conforms to the quality standards set forth in ISO 9001.

This instruction manual is intended to provide the user with all the information necessary to install, operate and maintain the Quantim[®] QMC Series Mass Flow Meters and Controllers.

Description

Quantim® QMC Series Mass Flow Meters and Controllers for gases and liquids are used to provide accurate measurements of fluid flow, fluid density and temperature. The heart of these instruments is the Coriolis mass flow sensor, which produces an electrical output signal directly proportional to mass flow rate and density. Quantim® Mass Flow Controllers couple the Coriolis sensor with a control valve. Additionally, Quantim® Mass Flow Controllers possess digital signal processing (DSP) electronics and PID control electronics to provide measurement and control in one complete package.

Quantim® is available for a wide range of gas and liquid flows.

(See specifications, Section 1 for details).

Brooks Instrument

Section 1 Introduction

Performance Specifications

Table 1-1 Product Specifications

	iodiione	QMCC (Controller)			QMCM (Meter)	
Performance	2	2	4	2	2	4
Tube Size:	2	3	4	2	3	4
Nominal Flow Range ¹ :						
Liquid (kg/hr):	0.15	0.78	7.97	0.19	1.30	13.50
Gas (kg/hr):	0.076	0.214	1.796	0.103	0.53	3.840
Gas (sccm) ² :	1051	2955	24787	1432	7207	53116
Maximum Flow Liquid (kg/hr) ¹ :	0.3	1.4	16.0	0.38	1.4	27.0
Minimum Flow Liquid (kg/hr):	0.001	0.010	0.100	0.001	0.010	0.100
Flow Accuracy ^{3,4} :	Star	ndard Flow Accuracy	-		ate, whichever is greater	
Standard Flow Accuracy:			Liquid Gas: 0.59			
Zero Stability Stainless Steel Sensor (kg/hr):	0.00013	0.0010	0.0040	0.00013	0.0010	0.0040
Repeatability & Reproducibility:		+0.05% or +[0.5 x	(zero stability/flowra	te) x 100]% of rate v	vhichever is greater	
Response Time (Settling Time): 2% F.S. of final value, (per SEMI Guideline E17-91)		<2 seconds			<0.5 seconds	
Temperature Coefficient			Zero: 0.05 Span: 0.03			
Control Range / Turndown ⁵			100:1 or down t	o minimum flow		
Ratings						
Operating Temperature Range ⁶ :			0 to	60°C		
Temperature Accuracy (Device):			±0.	5°C		
Differential Pressure Range:	Liquid: 10 to 200 psi (0.69 to 13.8 bar) Gas: 10 to 150 psi (0.69 to 10.3 bar)					
Maximum Operating Pressure:	Standard: 500 psi (34.5 bar) Optional: 1500 psi (103 bar)					
Density Range:	0 to 2.0 g/cc					
Density Accuracy ⁷ :	±0.005 g/cc					
Leak Integrity (External):	Elastomer: Outboard 1 x 10 ⁻⁹ atm. cc/sec., helium (max) Metal Seal: 1 x 10 ⁻¹⁰ atm. cc/sec., helium (max)					
Mechanical						
Materials of Construction (Process Wetted):		316L, 3	16L VAR, High alloy	ferritic stainless and	17-7PH	
Materials of Construction (Process Seals):	316L, 316L VAR, High alloy ferritic stainless and 17-7PH Elastomer Seal: Viton® fluoroelastomers, Buna, Kalrez® or EPDM Metal Seal: stainless steel and nickel					
Housing:			IP40: polyurethane	•		
In-Line Filter ⁸ :			controller: 1 micron oze 3 or 4: 10, 20, 30	or 10 micron filter re		
Weight:		1400 31	IP40: 2.4 k	g (5.4 lbs.)	Number 2	
Moisture Content:	IP66: 2.5 kg (5.6 lbs.) Purged to exhaust dew point less than -40°C (-40°F) prior to shipment to remove calibration liquid, to prevent process contamination. Then vacuum bagged at ambient					
Process Fitting Options:	room conditions. Elastomer Seal: 1/16", 1/8", 1/4" or 6mm tube compression, 1/8" or 1/4" NPT(F), 1/8" or 1/4" VCR, 1/4" VCO Metal Seal: 1/8" VCR, 1/4" VCR, 3.2 mm UPG					
Electrical Connections:	IP40: 15 pin D-Type connector (See Figure 5) IP66: 15 conductor terminal block (26-20 Awg) (See Figure 6)					
Dimensions:					<u> </u>	
Vibration:	(See Figures 1 through 4) Tested per: IEC 60068-2-64 Ed 2.1, Table A.3, Category 1, per ETSI EN 300 019-2-3, T 3.2., 30 min / axis, 1.1m/s2 (0.1g), 5 to 100Hz IEC 60068-2-6, Table A.1, 75min / axis, Peak Acceleration of 9.8m/s2 (1g), 5 to 2,000Hz, 5 Sweeps					

Table 1-1 Product Specifications (Contin.)

Diagnostics	QMCC (Controller)	QMCM (Meter)	
Diagnostics Status Lights:	Status and A	Narm LEDs	
Alarms:	Mass Flow, Density, Volumetric Flow, Temperature, Slug Flow, Diagnostic Failure, Setpoint Deviation, Valve Drive		
Electrical			
Output Signal:	Digital: RS485 S-Protocol (See RS485 Supplemental Manual – QMC for additional details) Analog: Primary: 0-20 mA, 4-20 mA, 0-5 Vdc, or 0-10 Vdc active output represents mass flow or volume flow(3) Secondary: 0-20 mA, 4-20 mA 0-5 Vdc or 0-10 Vdc active output represents density or temperature. Alarm output, max. voltage 30 Vdc, max. current 100 mA		
Input Signal:	Digital: RS485 S-Protocol (See RS485 Suppler Analog: Command (setpoint): 0-20 mA, 4-20 Valve Override (VOR) Function: Left floating/unconnected - instrument contro Connected to signal at or above 5.0 volts - va Connected to signal at or below 0.0 volts - va	mA, 0-5 Vdc or 0-10 Vdc ols flow at setpoint lve is forced open	
Power Requirements:	Voltage: +14	to 27 Vdc	
Nominal Current:	Controller: 165mA @ 2 Meter: 80mA @ 27V		
Max Current:	Controller: 760 Meter: 260m		
Max Power	Controller: 10.6 W @ 14 Vdc Meter: 3.7 W @ 14 Vdc		
Additional Functions & Outputs			
Damping:	Factory set time constan	t from 0 to 10 seconds	
LED's:	'STAT' solid green: system operative 'AL' solid red: system fault		
Pushbuttons:	'ZERO' setting pushbutton		
Approvals, Certifications & Compliance			
Environmental Compliance:	EMC Directive 2014/30/E ROHS Directive 2011/		
Pressure Effects Compliance:	Pressure Equipment D "Sound Enginee		
Additional Certifications (Optional):	Material 2.1 EN10204, Material 3.1B Oxygen Clean, Certific		
IP4x Series: UL Recognized E73889, Vol 3, Section 3. Non Incendive, Class I Division 2 Groups A, B, C and D; T4 per UL 1604, UL 508, and CSA 22.2 No. 213 1987; C-22.2 No. 14-M91, Ex nC IIC T4 per CSA E79-1 IP6x Series: UL Recognized E73889, Vol 1, Section 26 (conduit entry) Non Incendive, Class I Division 2 Groups A, B, C and D; Dust Ignition-Proof, Class II, Division 2, Groups F and G; Suitable for Class III, Division 2, T4 per UL 1604, UL 508, and CSA 22.2 No. 213 198 C-22.2 No. 14-M91, Ex nC IIC T4 per CSA E79-15, Class 1, Zone 2, AEx nC IIC T4 per ANSI/UL 60079-15 IECEX DEK 24.0063X, Ex ec IIC T4 Gc, Ex tc IIIC T135 °C Dc DEKRA 25ATEX0013X, II 3 G Ex ec IIC T4 Gc, II 3 D Ex tc IIIC T135 °C Dc IEC 60079-0: 2017 (Ed. 7), IEC 60079-7: 2017 (Ed. 5.1), IEC 60079-31: 2022 (Ed. 3) EN IEC 60079-0: 2018 + A11: 2024, EN 60079-7: 2015 + A1:2018 + A11: 2024,		Induit entry) , C and D; ss F and G; 14, UL 508, and CSA 22.2 No. 213 1987; 9-15, 0079-15 IC T135 °C Dc II 3 D Ex tc IIIC T135 °C Dc (Ed. 5.1), IEC 60079-31: 2022 (Ed. 3)	
	EN 60079-31:2014		

Note: Not all certifications are available for all QMC specifications and configurations. See page 4 for additional installation instructions and conditions of use.

Brooks Instrument Section 1 Introduction

Notes

- The nominal flow rate is the flow rate at which water at reference conditions causes approximately 1 bar of pressure drop or the laminar to turbulent transition flow whichever is lower. Maximum flow rate is higher than the nominal flow rate and is dependent upon process fluid and process conditions.
- ² Standard volumetric conditions are 14.696 psia and 70°F.
- 3 Actual volumetric flow is a function of the mass flow and the density measurements; therefore the accuracy of actual volumetric flow is a function of the mass flow and density accuracy.
- ⁴ Accuracy includes combined repeatability, linearity, hysteresis and calibration system uncertainty. Specifications are based on reference test conditions of water/nitrogen at 68 to 77°F (20 to 25°C) and 15 to 30 psig (1 to 2 bar).
- ⁵ Control range for QMCC controller is 100:1 due to control valve leakby. Turndown for QMCM meter is only limited by acceptable accuracy at low end of flow range and may be greater than 100:1
- ⁶ A temperature rise of up to 10°C (68°F) from internal heating can occur in an open environment where ambient temperature is 23°C (73°F). The device temperature is affected by the ambient and process temperature as well as warming when the device is powered. The device should be maintained in the specified temperature range at all times.
- ⁷ The density measurement at temperatures other than 25°C (77°F) has an additional error of approximately 0.000125 grams/cc per °C.
- Additional upstream filtration is always recommended to remove any particulate from the process fluid before it flows through these devices. In most applications, Brooks in-line filters are recommended as a secondary filter in addition to other upstream filtering methods. The use of Brooks in-line filters are not recommended in moisture sensitive applications.

WARNING

Do not operate this instrument in excess of the specifications listed below. Failure to heed this warning can result in serious personal injury and or damage to the equipment.

A CAUTION

It is the user's responsibility to select and approve all materials of construction. Careful attention to metallurgy, engineered materials and elastomeric materials is critical to safe operation.

WARNING

WARNING: EXPLOSION HAZARD - Do not open device enclosure or disconnect equipment when an explosion atmosphere is present.

WARNING

EXPLOSION HAZARD – Substitution of any components may impair suitability for Class I, Division 2.

IECEx and ATEX Special Conditions:

- 1. The equipment shall only be used in an area of not more than pollution degree 2, as defined in IEC 60664-1.
- 2. Provisions shall be made to prevent the rated voltage from being exceeded by transient disturbances of more than 119 V.
- 3. Connectors are not to be used during operational maintenance and may only be disconnected or connected when the system supply is switched off or when the location is confirmed to be non-hazardous.
- 4. Equipment shall be installed in areas of low risk to mechanical impact.
- 5. After wire termination, replace top lid and torque top lid screws to 8 in-lbs.

UL Listed Installation Instructions:

- 1. The hazardous locations classes, groups and division as described under products covered.
- $2. \ To \ maintain \ Ingress \ Protection \ (IP) \ rating, \ zero \ screw \ and \ diagnostic \ port \ screw \ must \ be \ installed.$
- 3. The equipment shall only be used in an area of not more than pollution degree 3, as defined in IEC 60664-1.
- 4. Evaluated for low risk of mechanical danger.
- 5. Transient protection shall be provided that is set at a level not exceeding 140 % of the peak rated voltage value at the supply terminals to the equipment.
- 6. To minimize risk from electrostatic discharge, only clean the device with a damp cloth.
- 7. After wire termination, replace top lid and torque top lid screws to 8 in-lbs.

$\label{eq:ull_problem} \mbox{UL Recognized versions of QMC - Conditions of Acceptability:} \\$

- 1. These devices are to be used within their ratings.
- 2. These devices are to be mounted in a suitable enclosure in the end product rated not less than IP54.
- 3. The wiring terminals are suitable for field wiring.
- 4. The suitability of the wiring method is to be determined in the end-use application.
- 5. These devices are intended to be powered by a class 2 power source.
- 6. These devices were evaluated for use in a maximum ambient temperature of 60°C.
- 7. The equipment shall only be used in an area of at least pollution degree 2, as defined in IEC 60664-1.
- 8. Transient protection shall be provided that is set at a level not exceeding 140 % of the peak rated voltage value at the supply terminals to the equipment
- 9. Evaluated for low risk of mechanical danger
- 10. To minimize risk from electrostatic discharge, only clean the device with a damp cloth
- 11. After wire termination, replace top lid and torque top lid screws to 8 in-lbs.

Dimensions

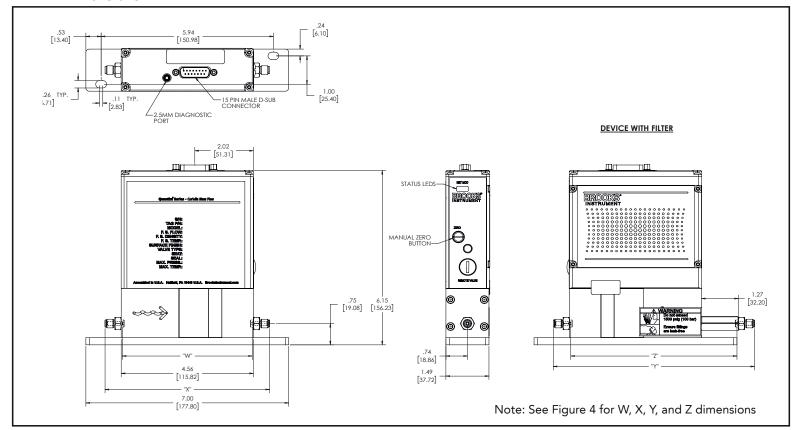


Figure 1-1 Dimensional Drawing QMC IP40

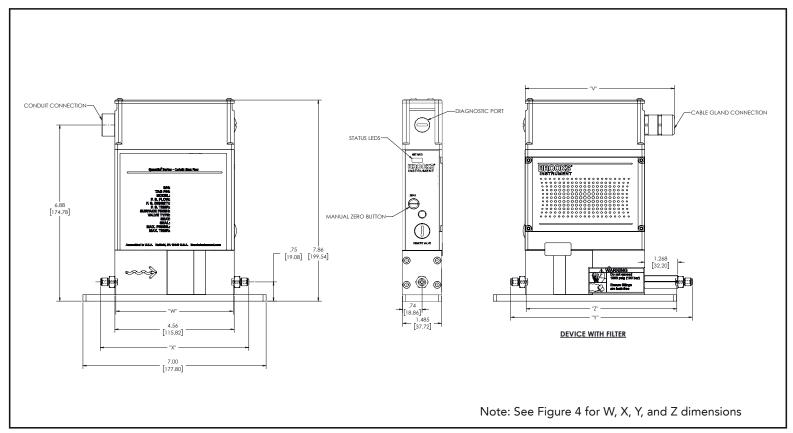


Figure 1-2 Dimensional Drawing QMC IP6x / Class 1 Division 2 Zone 2

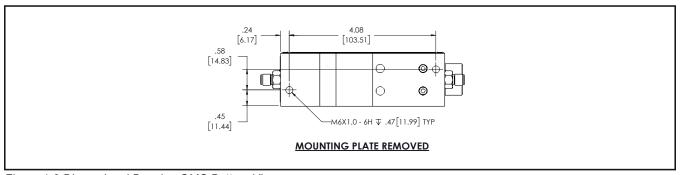


Figure 1-3 Dimensional Drawing QMC Bottom View

FITTING	"W" DIMENSION (NO FILTER)	"X" DIMENSION (NO FILTER)	"Y" DIMENSION (FILTER)	"Z" DIMENSION (FILTER)
1/8" VCR	N/A	5.92 [150.37]	7.19 [182.57]	N/A
1/4" VCR	N/A	6.64 [168.66]	7.91 [200.86]	N/A
1/16" TUBE COMPRESSION	5.30 [134.62]	5.68 [144.27]	6.95 [176.47]	6.57 [166.88]
1/8" TUBE COMPRESSION	4.49 [114.05]	5.68 [144.27]	6.95 [176.47]	5.76 [146.30]
1/4" TUBE COMPRESSION	5.30 [134.62]	5.92 [150.37]	7.19 [182.57]	6.57 [166.88]
6mm TUBE COMPRESSION	5.31 [134.87]	5.93 [150.62]	7.2 [182.82]	6.58 [167.13]
1/8" NPT	N/A	5.81 [147.57]	7.08 [179.77]	N/A
1/4" NPT	N/A	6.19 [157.23]	7.46 [189.43]	N/A
1/4" VCO	N/A	6.14 [155.96]	7.41 [188.16]	N/A
3.2mm UPG	N/A	5.92 [150.3]	N/A	N/A

NOTE: "W" & "Z" dimension reflects length of internal tube locating shoulder of each fitting.

Figure 1-4 Lay-In Dimensions Integral Valve

 $\bigcirc \begin{pmatrix} 1 & 0 & 0 & 0 & 0 & 0 & 0 & 0 \\ 9 & 0 & 0 & 0 & 0 & 0 & 0 & 15 \end{pmatrix} \bigcirc$

Pin	Function	Controller	Mete
1	Setpoint Common	*	N/A
2	0-5(10) Volt Flow Output	*	*
3	(TTL) Open Collector Alarm Output	*	*
4	(0)4-20 mA Flow Output	*	*
5	Power Supply (14-27 V)	*	*
6	Not Connected	N/A	N/A
7	(0)4-20 mA Setpoint Input	*	N/A
8	0-5(10) Volt Setpoint Input	*	N/A
9	Power Common	*	*
10	Signal Out Common	*	*
11	Not Connected	N/A	N/A
12	Valve Override Input	*	N/A
13	Density or Tempertaure output, Current or Voltage	*	*
14	RS-485, B(-) Input/Output	*	*
15	RS-485, A(+) Input/Output	*	*

Figure 1-5 D-Connector Electrical Pin Connections

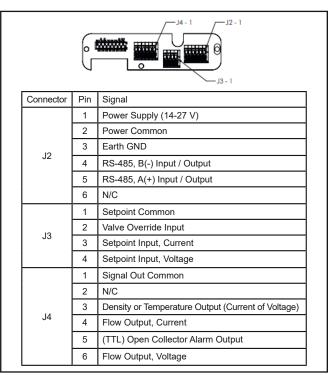


Figure 1-6 Terminal Block Pinout Connections for IP66 or Class 1 Division 2 / Zone 2

General

WARNING

Operating Procedure: Do not operate this instrument outside the specifications listed in Section 1. Before bringing the unit into operation, make sure that all fluid connections have been correctly tightened and that all necessary electrical connections have been made.

Receipt of Equipment

When the equipment is received, the outside packing case should be checked for damage incurred during shipment. If the packing case is damaged, the local carrier should be notified at once regarding their liability. A report should be submitted to Brooks Instrument. Visit the Brooks Instrument website at www.brooksinstrument.com/en/service-support

Remove the envelope containing the packing list. Carefully remove the instrument from the packing case. Make sure spare parts, accessories and documentation are not discarded with the packing materials. Inspect for damaged or missing parts.

Recommended Storage Practice

If intermediate or long-term storage is required, it is recommended that the instrument be stored in accordance with the following:

- a. In the original vacuum bag and shipping container.
- b. In a sheltered area with the following conditions: Ambient temperature 70°C (160°F) maximum and 0°C (32°F) minimum.
- c. Relative humidity 45% nominal, 60% maximum, 25% minimum.

Upon removal from storage a visual inspection should be conducted to verify the condition of equipment is "as received".

Return Shipment

Prior to returning any instrument to the factory for any reason, visit our website for instructions on how to obtain a Return Materials Authorization Number (RMA#) and complete a Decontamination Statement to accompany it: www.brooksinstrument.com/en/service-support. All instruments returned to Brooks also require a Material Safety Data Sheet (MSDS) for the fluid(s) used in the instrument. Failure to provide this information will delay processing of the instrument.

Instrument must have been purged in accordance with the following:

WARNING

Before returning the device, purge thoroughly with a dry inert gas such as Nitrogen before disconnecting process connections. Failure to correctly purge the instrument could result in fire, explosion or death. Corrosion or contamination may occur upon exposure to air.

Transit Precautions

To safeguard against damage during transit, transport the instrument to the installation site in the same container used for transportation from the factory if circumstances permit.

Fluid Connections

General Mounting Practices

Use good piping practices to minimize transmitting any torque or bending loads onto the process connections on Quantim[®]. Always verify there are no leaks prior to starting Quantim[®] on process fluid. The instrument is delivered from the factory with a rigid surface mounting plate. For optimum performance, this mounting plate should be used to mount Quantim[®] to a rigid surface. If panel mounting is required, the bottom of the instrument is provided with two M4 and M6 (see dimensional drawings, Section A) mounting holes to properly install the instrument on a rigid flat plate. Panel mounting is not recommended for Quantim[®] flow controllers with remote valve configuration.

WARNING

Any rotation of the inlet or outlet fitting during installation of a metal seal device may result in a leak. Always use two (2) wrenches when attaching gas lines to prevent rotation.

Mechanical Installation

Prior to installation:

- a. Verify that tube fittings match the fitting type and size supplied with your Quantim[®] instrument.
- b. Make certain that all piping and fittings are clean and free of obstructions for the instrument and filter.
- c. Assure that the final installation permits easy access to the instrument. (For Dimensional Drawings see Section 1)

A CAUTION

When installing the Mass Flow device, care should be taken to prevent foreign materials from entering the instrument's inlet or outlet. Internal passages are very small. It is recommended that an inlet filter be used to limit the chance of clogging. Do not remove the protective end-caps until the actual moment of installation. When used with reactive fluids (some of which may be toxic or moisture sensitive), contamination or corrosion may occur as a result of plumbing leaks or improper purging. Plumbing should be checked carefully for leaks. Care must be taken to thoroughly purge / dry down the system before introduction of any moisture sensitive process fluid.

Recommended installation procedures:

- a. All models should be mounted to a stable surface that is relatively free from mechanical shocks and mechanical vibration using the supplied mounting plate.
- b. Leave sufficient room for access to the electrical connections.
- c. Install in a manner that allows the instrument to be easily removed.
- d. Install the instrument with an appropriate filter on the fluid inlet side.
- e. It is recommended that a positive shutoff valve be installed downstream of the Quantim[®] to allow for proper zeroing after installation.

CAUTION

The control valve of the Quantim Mass Flow Controller provides precision control and is not designed for positive shutoff. If positive shutoff is required, it is recommended that a separate shut-off valve be installed in-line, downstream from the Quantim Mass Flow Controller.

A CAUTION

If the power supply to the Quantim Mass Flow Controller is interrupted, a NORMALLY CLOSED valve will be fully closed. However, a shutoff valve is recommended if the process architecture requires it as the Quantim control valve may not provide positive shutoff.

▲ WARNING

To prevent ignition of hazardous atmospheres disconnect supply circuits before opening. Keep cover tight when in operation. Conduit runs must have seal fittings installed within 3 inches of enclosure

Process Mounting

Quantim® will function in any orientation if the Coriolis sensor and the control valve remain filled with process fluid. Entrapped gas in a liquid application and entrapped liquid in a gas application should be prevented as it may disturb the Coriolis sensor and the control valve. Install Quantim® considering the direction of the FLOW arrow. The arrow indicating proper flow direction is engraved on the instrument between the process fittings. (See Figure 2-1 below.)

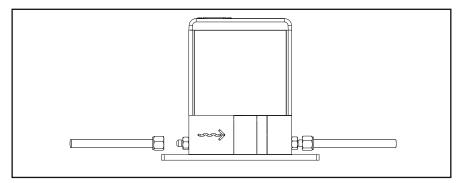


Figure 2-1 Flow Direction Through the Quantim, as Indicated by the Arrow Engraved on the Meter/Controller Body.

Horizontal Mounting

If installing Quantim[®] in a horizontal orientation, liquids should flow in the direction of the flow arrow. Situations of entrapped gas in the liquid process should be avoided. In liquid flow applications, it is recommended to mount Quantim[®] in an inverted attitude on the underside of the pipe to limit the possibility of entrapped gas collecting in the sensor, which can cause errors (See Figure 2-2).

For use in gas flow measurement, Quantim[®] should be mounted on the topside of the pipe to limit the possibility of entrapped fluid collecting in the sensor, which can cause errors. (See Figure 2-3).

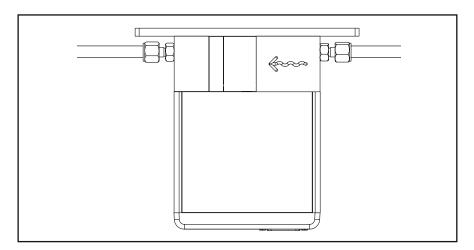


Figure 2-2 Horizontal Inverted Installation

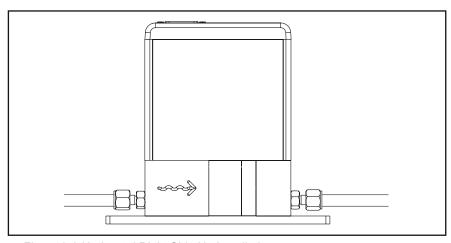


Figure 2-3 Horizontal Right Side Up Installation

Vertical Mounting

If Quantim® is installed in a vertical orientation, for use in a liquid application, liquid should flow upwards through the instrument to help minimize errors due to entrapped gas (See Figure 2-4). For gas flow vertical orientation, flow up or down is acceptable.

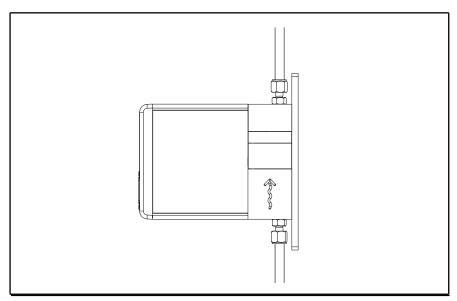


Figure 2-4 Vertical Flow Up Installation

Electrical Interfacing

Meter and Controller

Flow Output (IP40: Pins 2, 4 and 10 or IP6x: J4-6, J4-4 and J4-1)

Flow Output configuration is a factory selected option.

Each Quantim® instrument is calibrated as either 0-5 (10) Vdc or (0) 4-20 mA at the factory as specified when ordering. Pin 2 (J4-6) indicates the flow rate, represented by a 0-5 (10) Vdc signal proportional to flow, if so configured. Recommended load on Pin 2 (J4-6) is >1K ohm. Pin 4 (J4-4) indicates the flow rate, represented by a (0) 4-20 mA signal current proportional to flow, if so configured. Maximum series resistance on Pin 4 (J4-4) is 500 ohms. Do not apply power to Pin 4 (J4-4). The current and voltage signals are returned via Pin10 (J4-1).

Analog Setpoint Input (IP40: Pins 7, 8 and 1 or IP6x: J3-3, J3-4 and J3-1; Controller models only) Signal Input configuration is a factory selected option.

The Mass Flow Controller can be used either with a current or voltage set point as configured when ordered. If configured for current (4-20 mA or 0-20 mA) setpoint, connect the setpoint signal to Pin 7 (J3-3) and the setpoint return signal to Pin 1 (J3-1). Input impedance on Pin 7 (J3-3) is 250 ohms. Do not apply power to Pin 7 (J3-3). If configured for voltage (0-5 Vdc or 0-10 Vdc) setpoint, connect the setpoint signal to Pin 8 (J3-4) and the setpoint return to Pin 1 (J3-1). Input impedance to Pin 8 is 200K ohms.

Power Supply (IP40: Pin 5 and Pin 9 or IP6x: J2-1 and J2-2)

Both Mass Flow Meter and Controller models are connected via Pins 5 (J2-1) (+14 to +27 Vdc) and 9 (J2-2) (power supply common) on the customer connector. See Section 1, Performance Specifications for current requirement.

EMC note: The DC Input Port of the device is not intended to be connected to a DC Distribution Network; therefore the DC Input Leads were tested as I/O signal / control ports.

WARNING

With regard power supply connections, the user must ensure that the minimum required voltage and current is available at the mass flow device taking into consideration any losses in the interconnecting cable.

Valve Override (IP40: Pin 12 or IP6x: J3-2; Controller models only)

To open or close the control valve independently of the setpoint signal (e.g. for process reasons), Pin 12 (J3-2) is available to carry a valve override signal. Leave floating (i.e. not connected) to allow for normal control operation. Input impedance on Pin 12 (J3-2) is >50K ohms.

Valve Operation	Pin 12 (J3-2)
Normal Operation	Floating
Valve Open	> 5 Vdc
Valve Closed	0 VDC

Secondary Output, Density or Temperature (IP40: Pin 13 and Pin 10 or IP6x: J4-3 and J4-1)

Pin 13 (J4-3) indicates the density or temperature, represented by a (0) 4-20 mA or 0-5 (10) Vdc signal, proportional to density or temperature. The current and voltage signals are returned via Pin 10 (J4-1). Maximum series resistance on Pin 13 (J4-3) is 500 ohms when configured for (0) 4-20 mA. Recommended load on Pin 13 (J4-3) is >100K ohms when configured for 0-5 (10) Vdc. Do not apply power to Pin 13 (J4-3).

Alarm Output (IP40: Pin 3 and Pin 5 or IP6x: J4-5 and J2-1)

See Figure 2-5.

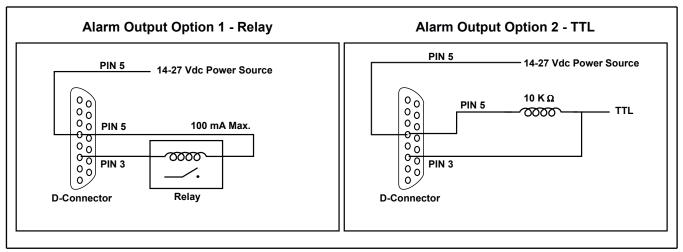


Figure 2-5 Alarm Output Wiring Options

Table 2-1 Electrical Interfacing for Quantim QMC IP40

Pin IP40 D-Con	Function	Controller	Meter
1	Setpoint Common	*	N/A
2	0-5(10) Volt Flow Output	*	*
3	(TTL) Open Collector Alarm Output	*	*
4	(0)4-20 mA Flow Output	*	*
5	Power Supply (14-27 V)	*	*
6	Not Connected	N/A	N/A
7	(0)4-20 mA Setpoint Input	*	N/A
8	0-5(10) Volt Setpoint Input	*	N/A
9	Power Common	*	*
10	Signal Out Common	*	*
11	Not Connected	N/A	N/A
12	Valve Override Input	*	N/A
13	Density or Temperature output, Current or Voltage	*	*
14	RS-485, B(-) Input/Output	*	*
15	RS-485, A(+) Input/Output	*	*

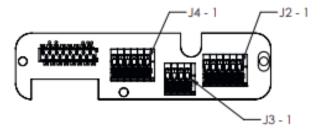


Table 2-2 Electrical Interfacing for Quantim QMC IP6x

Pin IP6x Connector	Pin	Signal
	1	Power Supply (14-27 V)
	2	Power Common
10	3	Earth GND
J2	4	RS-485, B(-) Input / Output
	5	RS-485, A(+) Input / Output
	6	N/C
	1	Setpoint Common
10	2	Valve Override Input
J3	3	Setpoint Input, Current
	4	Setpoint Input, Voltage
	1	Signal Out Common
	2	N/C
J4	3	Density or Temperature Output (Current of Voltage)
J4	4	Flow Output, Current
	5	(TTL) Open Collector Alarm Output
	6	Flow Output, Voltage

WARNING

When wiring terminal block in IP6x device, ensure wires are appropriate length and are properly dressed.

RS485 (S-Protocol) Communication

Quantim® Model QMC is equipped with RS485 communication capability. Refer to Figure 2-1 for IP40 or Figure 2-2 for IP6x, Electrical Interfacing for Quantim, to enable the device to communicate via a personal computer, PLC or DCS for process control. Baud rate selections for Quantim® with RS485 are: 1200, 2400, 4800, 9600, 19200 and 38400 baud. The device is factory set with a baud rate of 19200 and can be changed using the Brooks Expert Support Tool (BEST). The RS485 is a multidrop connection which allows a maximum of 32 devices to be connected to a personal computer or control system. Personal computers are not equipped with RS485 ports as standard. An RS232/USB to RS485 converter or RS485 interface board is therefore required to connect an RS485 network to a standard personal computer. The RS485 bus is a daisy chain network, meaning the wires are connected at the units as in Figure 2-6.

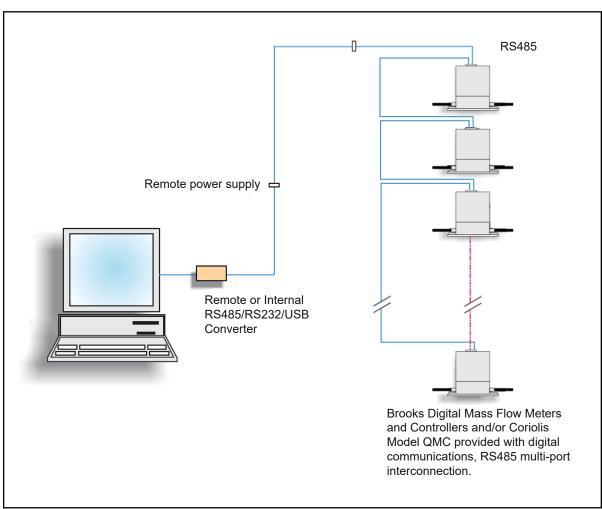


Figure 2-6 General Wiring

Interconnection with Peripheral Equipment

The following cables are available for connection of Quantim® Model QMC IP40 Meters and Controllers with 15 pin D connector to the Brooks Instrument Microprocessor Control & Read-out Unit: Models # 0152, 0154, 0251 or 0254

```
Length: 3ft (1m); part number 124Y054AAA
Length: 5ft (1.5m); part number 124Y050AAA
Length: 10ft (3m); part number 124Y051AAA
Length: 25ft (7m); part number 124Y052AAA
Length: 50ft (15m); part number 124Y053AAA
```

Or in case both Flow and Density or Temperature functions have to be made available: (for 4-20 mA secondary output only)

```
Length: 5ft (1.5m); part number 124Z906ZZZ
Length: 10ft (3m); part number 124Z907ZZZ
Length: 25ft (7m); part number 124Z908ZZZ
Length: 50ft (15m); part number 124Z909ZZZ
```

The following open frame cables are available for connection of Quantim® to any secondary electronic device.

```
Length: 5ft (1.5m);
                                124Z361AAA
                  part number
Length: 10ft (3m);
                                124Z362AAA
                  part number
Length: 25ft (7m);
                  part number
                                124Z363AAA
Length: 50ft (15m); part number
                                124Z435AAA
Length: 75ft (22m); part number
                                124Z876AAA
Length: 100ft (30m); part number
                                124Z868AAA
Length: 150ft (45m); part number
                                124Z757AAA
Length: 200ft (60m); part number
                                124Z773AAA
```

(See Figure 2-7 for Wire Color Code Diagram)

Diagnostic Cable Kits

Basic BEST/MultiFlo Kit (USB to 2.5 mm Cable Assembly)

part number 778Z010ZZZ

BEST/MultiFlo Kit with Profibus/RS485 Power Supply part number 778Z012ZZZ

Cable Shielding Earth

Cable requirements:

Compliance with EMC directive 89/336/EEC, requires that the equipment be fitted with fully screened signal cables with at least 80% shielding. The cable shielding should be connected to the D-connector's metal shell and have 360° shielding at both ends. The shielding should be connected to an earth ground.

QMC IP40 D-CON PIN	Color	Function	Controller	Meter
1	BLK	Setpoint Common	*	N/A
2	WHT	0-5 (10) Volt Flow Output	*	*
3	RED	(TTL) Open Collector Alarm Output	*	*
4	GRN	(0) 4-20 mA Flow Output	*	*
5	ORG	Power Supply (14-27 V)	*	*
6	BLUE	Not Connected	N/A	N/A
7	WHT/BLK	(0) 4-20 mA Setpoint Input	*	N/A
8	RED/BLK	0-5 (10) Volt Setpoint Input	*	N/A
9	GRN/BLK	Power Common	*	*
10	ORG/BLK	Signal Out Common	*	*
11	BLU/BLK	Not Connected	N/A	N/A
12	BLK/WHT	Valve Override Input	*	N/A
13	RED/WHT	Density or Temperature output, Current, or Voltage	*	*
14	GRN/WHT	RS-485, B(-) Input/Output	*	*
15	BLU/WHT	RS-485, A(+) Input/Output	*	*
	(Cable Assembly for 'D' Type Connector		

Figure 2-7 Wire Color Codes for 'D' Connector Assembly

Operating Procedure

CAUTION

Any sudden change in system pressure may cause mechanical damage to elastomer materials. Damage can occur when there is a rapid expansion of fluid that has permeated elastomer materials. The user must take the necessary precautions to avoid such conditions.

WARNING

Before operating the flowmeter, ensure all fluid connections have been properly tightened and, where applicable, all electrical connections have been properly terminated.

After the wiring cable has been connected, power can be supplied to the instrument. During initialization, the instrument remains in start-up mode for about 5 seconds. The START-UP mode is indicated by the alternately flashing red/green status LEDs on the Meter/Controller. LEDs are on the side of the instrument (See Figures 3-1 and 3-2).

Status LED

The Status LED, indicates the operation condition of the instrument. During start-up, the status LED blinks red/green once per second to indicate proper start-up operation of the meter/controller. Then a solid green is displayed to indicate proper function.

The status LED will be illuminated a solid green color for the meter/controller, indicating that the instrument is ready for operation.

If the status LED is illuminated a solid red color, a START-UP issue has been determined by the onboard diagnostic programs. This condition can only be cleared by cycling power to the instrument. If the issue persists, call Technical Service at Brooks Instrument.

Technical Service

Brooks Technical Service is available to assist with start-up if you experience issues you cannot solve on your own. You will be asked to provide the model code and serial number of your Brooks equipment, which will assist us in answering your questions. For telephone references, please visit our website www.brooksinstrument.com/en/service-support/contact-technical-services.

Zero Adjustment

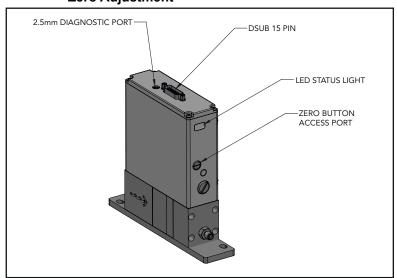


Figure 3-1 Location of the LEDs, Zero Button and Diagnostic Port, IP40 Device

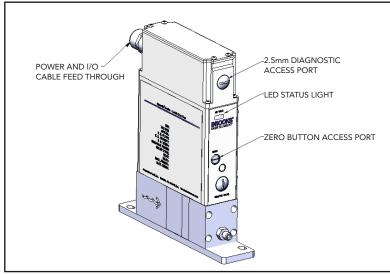


Figure 3-2 Location of LEDs, Zero Button and Diagnostic Port, IP6x Device

After Quantim® has been fully installed, you must perform the zeroing procedure. This procedure ensures that the instrument responds properly to zero flow condition and sets a baseline for flow. To perform the zeroing operation on the meter/controller, use the ZERO button, which is located on top right hand side (outlet side) of the instrument. Zero button must be pressed for at least 3 seconds to initiate zeroing procedure. Care should be taken when exercising the zero button. Ensure alignment of the tool on the zero button. Apply a small force to depress the button. NOTE: Excessive force may damage the zero button. The status LED will flash red on and off during the zeroing procedure. (See Figure 3-1 or Figure 3-2).

A CAUTION

After the instrument has been installed, you must perform the rezeroing procedure. A true zero flow condition must be present and the Coriolis sensor and control valve must both be completely full of process fluid during the re-zeroing procedure. This is done best by eliminating any pressure differential across the instrument. A shutoff valve, downstream from the instrument, is recommended to halt flow during the re-zeroing procedure.

Failure to zero the instrument after initial startup could cause measurement error.

Zero the instrument before putting the instrument in operation.

Zero Procedure

- 1. Prepare the instrument for zeroing:
 - a. Install the instrument according to the instructions in this manual.
 - b. Power-up sequence. Isolate device from flow pressure when applying power. Once the status indicator is illuminated green, pressure may be applied.
 - c. Apply power to the instrument and allow approximately 45 minutes to reach a stable condition.
 - d. Run the process fluid to be measured and controlled through the instrument until the temperature of the instrument approximates the normal process operating temperature. Use the Valve Override (V.O.R.) function to fully open the control valve to facilitate temperature stabilization.
- 2. Once the instrument has reached process temperature, close the external shutoff valve downstream from the instrument and wait for the flow to stop. Set the control function to zero and V.O.R. to normal once flow has stopped and all pressure differential across the instrument has been bled off.
- 3. Make sure that the instrument is completely filled with the process fluid under normal process conditions of temperature, pressure, density, etc. make sure there is no entrapped gas in the sensor tube and ensure a zero flow condition through the instrument.

A CAUTION

Flow through the instrument during zeroing procedure will result in an inaccurate zero setting.

Make sure fluid flow through the instrument is completely stopped during the zeroing procedure.

- 4. After confirming that fluid flow through the instrument is completely stopped, actuate the zero function as previously stated. Care should be taken when exercising the zero button. Ensure alignment of the tool on the zero button. Apply a small force to depress the button. NOTE: Excessive force may damage the zero button.
- 5. The default zero sample interval is 30 seconds. A successful zero operation on the controller and meter will be indicated by a solid green color status LED. A solid red color status LED indicates a failed zero process. A non-steady flash will indicate a failed condition. A failed condition can only be cleared by a power cycle.
- 6. Once the status LED turns green, zero process is complete and the instrument is ready for operation.

Please note that zero command will only be accepted when the output change is less than 1% of the maximum full scale of the device. This logic prevents an accidental zero command from being initiated when flow is present, through the device.

Calibration Procedure

Quantim[®] calibration is not described in this manual. If your Quantim[®] requires calibration, please visit our website www.brooksinstrument.com/en/service-support.

General

There are no routine maintenance procedures required to keep your Quantim® instrument in good operating condition. It is however, very important to keep the fluid entering Quantim® clean, and as a result periodic replacement of the inlet guard filter is recommended at a frequency determined by the cleanliness of the fluid. At a minimum this guard filter should be replaced annually.



WARNING

METER/CONTROLLER SEAL COMPATIBILITY

Products in this manual may contain metal or elastomeric seals, gaskets, O-rings or valve seats. It is the "user's" responsibility to select materials that are corrosion resistant and compatible with their process and process conditions. Using materials that are not compatible with the process or process conditions could result in the Meter or Controller leaking process fluid outside the pressure boundary of the device, resulting in personnel injury or death.

It is recommended that the user check the Meter or Controller on a regular schedule to ensure that it is leak free as both metal and elastomeric seals, gaskets, O-rings and valve seats may change with age, exposure to process fluid, temperature, and/or pressure.

WARNING

If it becomes necessary to remove the MFC/MFM from the system after exposure to toxic, pyrophoric, flammable or corrosive fluids, purge the flowmeter thoroughly before disconnecting the fluid connections. Failure to correctly purge the MFC/MFM could result in fire, explosion or death. Corrosion or contamination of the MFC/MFM upon exposure to air, may also occur.

A CAUTION

It is important that this MFC/MFM only be serviced by properly trained and qualified personnel.

Maintenance & Troubleshooting

System Checks

WARNING

Internal seals and component alignments are extremely critical within the device. Improper servicing of your Quantim can cause malfunction of the device and/or personal injury. This device <u>must</u> be serviced by factory personnel only. There are no customer serviceable components within the device. Disassembly of this device voids all warranties, explicit or implied.

Quantim® Mass Flow Meters and Controllers are typically used as a critical component in fluid systems. These systems can be complex in nature and therefore isolating a malfunction has to be done with a system perspective. An incorrectly diagnosed malfunction can cause many hours of unnecessary downtime. If possible, perform the following system checks before removing a suspect Mass Flow Meter or Controller for bench troubleshooting or return to the factory (especially if the system is new):

- 1. Identify a low resistance common connection and make sure that the correct power supply voltage and signals are present at the connector of the Quantim® device.
- 2. Verify that the process fluid connections have been made correctly, and that they have been tested for leaks.
- 3. If the Mass Flow Controller appears to be functioning but cannot achieve setpoint, verify that there is sufficient inlet pressure and pressure drop at the controller to provide the required flow.
- 4. Flow control instability can be a result of using Quantim® in a system that includes other active control elements such as pressure regulators. Depending on the tuning constants used in the Quantim® and the control dynamics of the other active elements, these devices can interfere with each other and cause flow instabilities. It is very important to take a complete system perspective when applying Quantim® to flow control applications.

Table 4-1 Maintenance & Troubleshooting

Observation	Cause	Resolution
Oscillating mass flow output can cause diagnostic alarm	Bubbles dissolved in the liquid. High pressure push gas can cause bubbles to disolve in fluid. Bubbles then form at the valve due to pressure drop, upsetting valve.	Use a degasser or use Helium as a push gas with 25-50ft. of Teflon® tube. Helium is a light gas and can permeate the Teflon tube to release bubbles.
	Oscillating pump pressure used to move the fluid. Piston action can cause pressure oscillations, upsetting valve.	Avoid using push gas. Use a pump or bladder tank to prevent head pressure.
	Pressure drop or inlet pressure deviates form calibrated values.	Pressure regulators on inlet and outlet of Quantim to stabilize pressure variations.
	Valve out of adjustment. Unstable inlet pressure.	Adjust pressure to original specifications.
	Defective PC board.	Contact Brooks Instrument. Check external pressure regulator.
	Valves are tuned digitally and mechanically for a particular △P.	Contact Brooks Instrument.
		Operate Quantim at specified pressure conditions.
Valve will not open or fully close	Valves are tuned digitally and mechanically for a particular ΔP . Proper valve response requires just the right amount of force to be applied by the valve. With too much or too little ΔP the valve will be mis-tuned.	Operate Quantim at specified pressure conditions. Check valve operation with the Brooks Service Tool.
	Mounting attitude is different from calibration attitude; Reason, gravity effects could pull valve open or closed.	Mount Quantim in the specified mounting attitude.
No Flow or unable to achieve full flow	Insufficient inlet pressure or pressure drop.	Adjust pressures, inspect in-line filters and clean/replace as necessary.
	Clogged Valve Orifice or Sensor.	Back flush the device with a solvent or purge gas with valve.

Table 4-1 Maintenance & Troubleshooting (continued)

Observation	Cause	Resolution
No Flow or unable to achieve full flow	Particulates in the flow stream.	Consider a larger orifice (valve stability could suffer).
	Agglomeration of fluid at orifice.	Institute regular PM back flushing.
	Chemical deposits.	Install proper filtration.
	Poor filtration of process fluid.	Contact Brooks Instrument.
	Valve out of adjustment (applicable to Controller).	
Valve out of adjustment	Valve guide spring failure (applicable to Controller).	Contact Brooks Instrument.
	Valve override input is grounded	Check the valve override input. (Pin12).
	Defective electronic board	Contact Brooks Instrument.
Output signal follows Setpoint at higher Setpoints but not at lower Setpoints	Control valve leaks or is stuck open.	Exercise the control valve alternating between valve override "open" and closed. If problem persists backflush the device with a solvent or purge gas with valve override "open".
Output signal stays in approx. 5.5 Vdc or 22 mA (regardless of setpoint) and	Valve leaks or is stuck open (applicable to Controller).	Backflush the device with a solvent or purge gas with valve override "open".
there is flow trough the meter/controller	+15 Vdc applied to the valve overrride input (applicable to Controller).	Check the valve override terminal (Pin 12). Contact Brooks Instrument.
	Defective PC board.	Contact brooks instrument.

Bench Troubleshooting

WARNING

If it becomes necessary to remove the instrument from the system power to the device is disconnected at the power supply.

WARNING

If it becomes necessary to remove the instrument from the system after exposure to toxic, pyrophoric, flammable or corrosive chemicals, purge the instrument thoroughly with a inert fluid such as water, alcohol, nitrogen, clean dry air or some other appropriate fluid before disconnecting the fluid connections. Failure to correctly purge the instrument could result in fire, explosion or death. The Quantim Mass Flow device may also become corroded or contaminated upon exposure to air.

Quantim Bench Testing (Refer to Figure 4-1)

- 1. Establish the proper electrical connection to the Quantim MFC/MFM. Do not connect the device to a fluid source yet.
 - a. Connect a +14 Vdc to +27 Vdc power supply to Pin 5 and power supply common to Pin 9.
 - b. Connect a voltage output signal read-out device (4-1/2 digit voltmeter recommended) onto Pin 2 (+) and Pin 10 (common).
 - c. If applicable, connect current output signal read-out device onto Pin 4 (+) and Pin 10 (common).
 - d. Switch on power and allow the instrument to stabilize.
 - e. In case of a MFC, adjust the setpoint input to zero.
- 2. Observe the output signal and if necessary, perform the zero adjustment procedure as outlined in Section 3-2.
 - a. Only perform the zero operations with the Coriolis Sensor filled with either 100% fluid or 100% gas at the appropriate pressures and ensure there is no fluid flowing through the device (differential pressure = 0 psi).
 - b. Connect the Quantim to a pressurized supply of inert fluid (for example high purity water). Fill the Quantim instrument completely taking care there is no entrained gas in the sensor and perform the zero operation as described in Section 3-2.
 - c. When applying Quantim to measure a gas, fill the sensor with an inert gas (nitrogen or clean dry air) at a pressure near the process operating pressure.
 - d. If the output signal does not zero properly, please contact Brooks Instrument for technical assistance.
- 3. For a MFC connect a 0-5 (10) Vdc source to Pin 8 and return to Pin 1 or connect (0) 4-20 mA source to Pin 7 and return to Pin 1.
- 4. Provide an electrical signal to the Quantim representing a setpoint of 50% of full scale flow and adjust the inlet and outlet pressures to calibration conditions.

- 5. Verify that the electrical output signal reaches 100% of flow. For MFC applications vary the setpoint over the 1% to 100% range and verify that the output signal matches the setpoint. If possible, connect a flow measurement device (such as a rotometer) to the Quantim outlet to monitor the actual flow behavior.
- 6. If the Quantim is functioning correctly, the problem may lie elsewhere in the flow system. Reverify the installation as well as the upstream/downstream fluid system configuration.
- 7. Please contact Brooks Instrument for further assistance visit our website www.brooksinstrument.com/en/service-support/contact-technical-services.

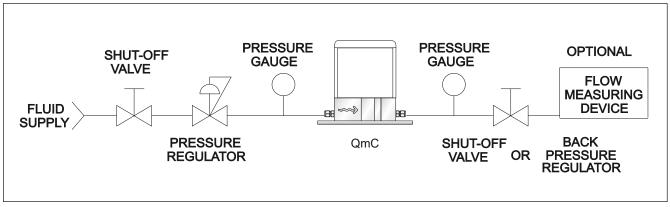


Figure 4-1 Bench Troubleshooting Circuit

LIMITED WARRANTY

Visit www.BrooksInstrument.com for the terms and conditions of our limited warranty.

BROOKS SERVICE AND SUPPORT

Brooks is committed to assuring all of our customers receive the ideal flow solution for their application, along with outstanding service and support to back it up. We operate first class repair facilities located around the world to provide rapid response and support. Each location utilizes primary standard calibration equipment to ensure accuracy and reliability for repairs and recalibration and is certified by our local Weights and Measures Authorities and traceable to the relevant International Standards.

Visit www.BrooksInstrument.com to locate the service location nearest to you.

START-UP SERVICE AND IN-SITU CALIBRATION

Brooks Instrument can provide start-up service prior to operation when required.

For some process applications, where ISO-9001 Quality Certification is important, it is mandatory to verify and/ or (re)calibrate the products periodically. In many cases this service can be provided under in-situ conditions, and the results will be traceable to the relevant international quality standards.

SEMINARS AND TRAINING

Brooks Instrument can provide seminars and dedicated training to engineers, end users and maintenance persons.

Please contact your nearest sales representative for more details.

Due to Brooks Instrument's commitment to continuous improvement of our products, all specifications are subject to change without notice.

TRADEMARKS

Brooks is a trademark of Brooks Instrument, LLC All other trademarks are the property of their respective owners.



Installation-Manual-Quantim-QMC-EN/541B234AAG/2025-06

Global Headquarters

Brooks Instrument 407 West Vine Street Hatfield, PA 19440-0903 USA Toll-Free (USA): 888-554-FLOW T: 215-362-3500

BrooksAM@BrooksInstrument.com

A list of all Brooks Instrument locations and contact details can be found at www.BrooksInstrument.com

