

4800 Series

Ultra-fast Responding, Compact, Thermal Mass Flow Controllers & Meters

The 4800 Series of mass flow controllers and mass flow meters features a broad flow range, compact size, a variety of analog and digital I/O options, a MEMS-based sensor that provides lightning fast response times, and many other benefits for a variety of applications. Fully RoHS compliant, the 4800 Series is an excellent choice for measurement and control of many common gases including air, N₂, O₂, Ar, He, H₂, CO₂, CO, N₂O, CH₄, C₃H₆ (Propene), and C₃H₈. The optional Local Operator Interface (LOI) provides a convenient user interface to view, control, and configure the 4800 Series devices eliminating the need for remote secondary electronics.



Features

Fast Response Time

Compact Size

Optional Local Operator Interface (LOI)

Low Pressure Drop Across the Sensor

Variety of Analog and Digital I/O

Fully RoHS Compliant

Benefits

Ensures rapid step during process recipe changes

Reduces space and eases installation

Provides a turnkey solution for local indication, set point control and device configuration eliminating the need for remote secondary electronics

Provide flow measurement with minimal pressure budget

Easily aligns with user requirements

Meets emerging environmental requirements

Product Specifications

Performance

| | |
|-------------------------|-----------------------------------------------------------------------------------------------------------------------------|
| Full Scale Flow Range | 50 ml/min - 40 l/min (50 sccm - 40 slpm) (N ₂ eq., at 0°C Ref, with typical 50 psid pressure differential) |
| Control Range | 2 - 100% |
| Flow Accuracy | ±3.0% of F.S., ±1.0% F.S. optional |
| Flow Repeatability | ±0.15% of F.S. |
| Response Time | Flow Signal: <0.3 sec Flow Control: Settling time <0.75 sec from 0 to 100% F.S. (typical <0.5 sec for all steps) |
| Temperature Coefficient | ±0.1% of F.S./°C (N ₂) |

Ratings

| | |
|-------------------------------------------|-----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Gases | Air, N ₂ , O ₂ , Ar, He, H ₂ , CO ₂ , CO, N ₂ O, CH ₄ , C ₃ H ₆ (Propene), C ₃ H ₈ (other gases upon request) |
| Operating Limits | Pressure 0 - 10 barg (0 - 150 psig) Temperature 0 - 50°C Humidity 5 to 95% R.H. (ambient) |
| Differential Pressure Range (Controllers) | 2000 Torr |
| Leak Integrity | 45 psid max |

Mechanical

| | |
|---------------------------|---------------------------------------------------------------------------------------------------|
| Materials of Construction | Wetted parts: stainless steel, fluoroelastomers, silicon-based sensor |
| RoHS | Fully RoHS compliant per EU Directive 2011/65/EU |
| Outline Dimensions | Refer to Figures 6 and 7 |
| Process Connections | Inlet/Outlet threads: 9/16" - 18 UNF threads, Refer to Figure 6 for available process connections |

Electrical



| | | | | | |
|-----------------------------------|--------------------------------------------------------------------------------------------------------|--------------|----------|--------------|----------|
| Electrical Connections | 15-pin D-sub connector Analog/RS232: 15-pin D-sub connector | | | | |
| Power Supply Voltage ¹ | +15 Vdc + 10% or +24 Vdc + 10% Device only uses single sided power supply Inrush current: <1A | | | | |
| Power Requirements | Model Device | 15 Vdc | | 24 Vdc | |
| | Type | Typical (mA) | Max (mA) | Typical (mA) | Max (mA) |
| | 4850 Controller | 130 | 160 | 150 | 200 |
| | 4860 Meter | 30 | 60 | 30 | 60 |
| Analog Input / Output | 0-5 Vdc or 4-20 mA | | | | |
| Digital Input / Output | RS232 (Standard with all analog I/O options) | | | | |
| Valve Override Signal | Valve Controller: Input Open Valve Closed: <0.3 V; open valve: >4.8 V | | | | |

Local Operator Interface (LOI)

| | |
|---------------------------|----------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------------|
| Display | Effective display area: 28mm wide, 11mm high Display Contents: 8x2 dot matrix display |
| Operating Limits | Temperature 0 - 50°C Operating Humidity 5 to 95% R.H. (ambient) |
| Electrical Connections | 2 15-pin D-sub connectors, one for the connection to the 4800 Series and one for the remote connection |
| Power Supply Voltage | The LOI optionally includes a wall mount power adaptor with a 3.5-mm DC-plug. The adaptor works with input voltages of AC 90-240 V/47-63Hz. The adaptor supports European, U.K., Australia and U.S. wall plugs. Power can also be supplied by a remote connection via the D-connector. |
| Materials of Construction | Enclosure: ABS plastic with CU-Ni plating |
| RoHS | Fully RoHS compliant per EU Directive 2011/65/EU |
| Outline Dimensions | Refer to Figure 8 |

¹ For high flows and/or low differential pressures (using orifices 0.049" (1.25mm) or 0.079" (2.0mm)) only 24 Vdc power is available.


4800 Series - Standard Process Connections

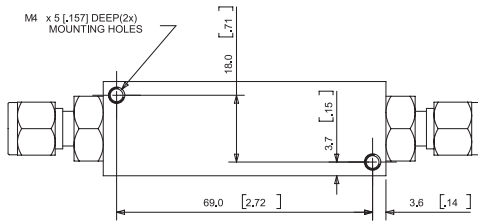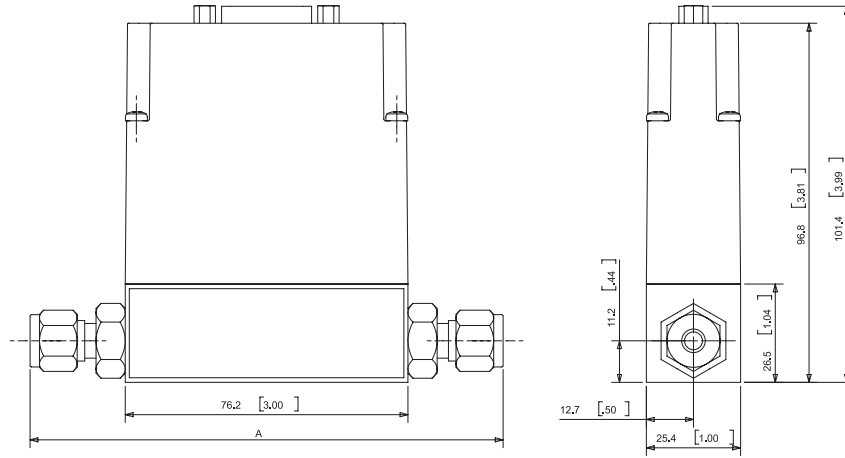


| Connections | Dim A |
|----------------------------------------------|---------------|
| 1/4" Tube Compression | 127.5 [5.02"] |
| 1/8" Tube Compression | 122.9 [4.84"] |
| 3/8" Tube Compression | 130.6 [5.14"] |
| 1/4" VCO | 115.8 [4.56"] |
| 1/4" VCR | 124.0 [4.88"] |
| 1/4" NPT-F | 116.4 [4.58"] |
| 1/4" RC-F | 116.4 [4.58"] |
| 6mm Tube Compression | 127.6 [5.02"] |
| 10mm Tube Compression | 131.0 [5.16"] |
| 1/4" Tube Compression for 5850TR Replacement | 128.8 [5.07"] |

mm [inches]

4800 Series - Downport Connections

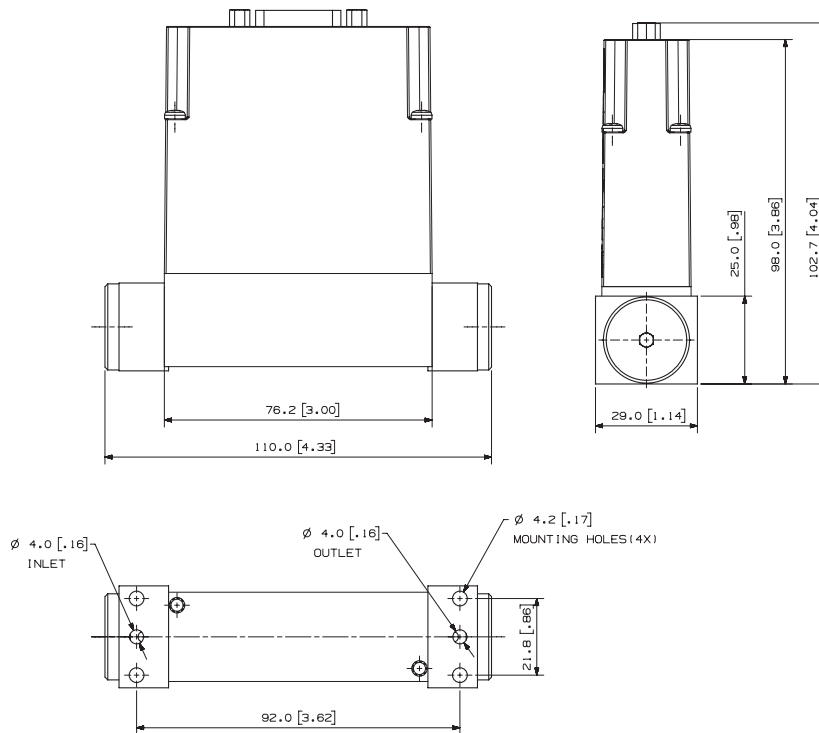


4800 Series - LOI Module

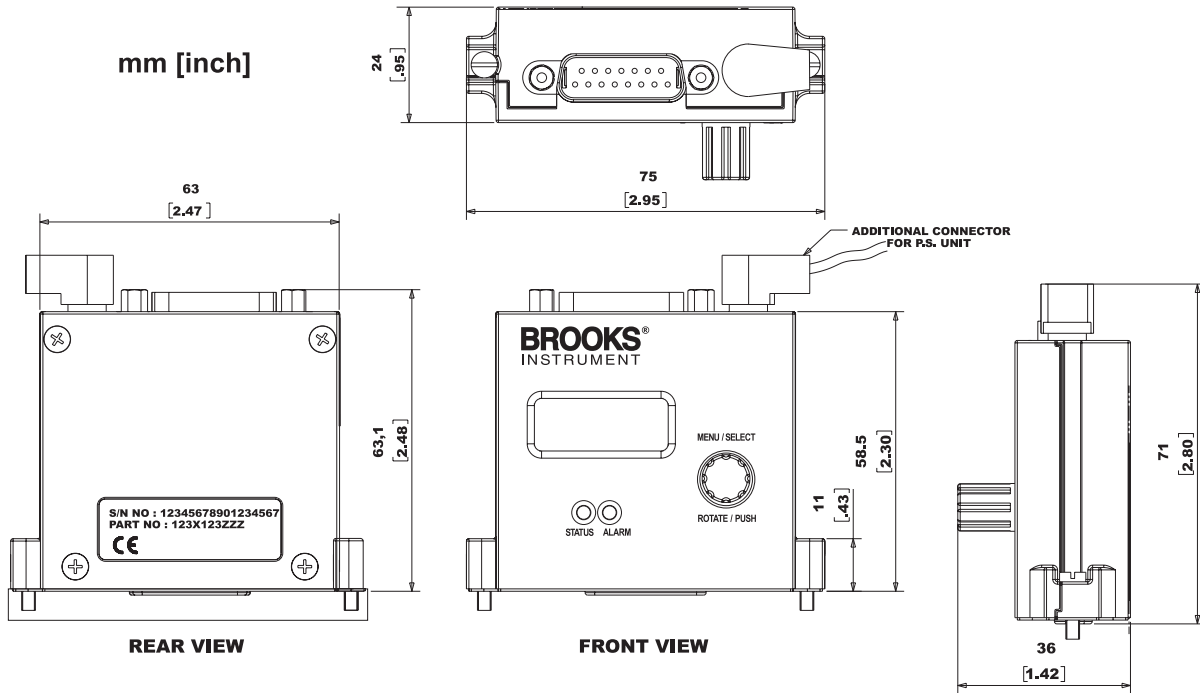




4800 Series - Pin-Out Diagram

15 Pin D-Sub Connector



| Pin | 4800 Series / LOI |
|-----|-------------------------|
| 1 | Setpoint Signal Common |
| 2 | Flow Voltage Output |
| 3 | No Connection |
| 4 | Flow Current Output |
| 5 | Positive Supply Voltage |
| 6 | No Connection |
| 7 | Setpoint Current Input |
| 8 | Setpoint Voltage Input |
| 9 | Power Supply Common |
| 10 | Flow Signal Common |
| 11 | No Connection |
| 12 | Valve Override Input |
| 13 | No Connection |
| 14 | RXD |
| 15 | TXD |

These certifications cover the 48xx Series thermal mass flow devices as well as the Local Operator Interface (LOI).

| Mark | Agency | Certification/ Marking/ Directive | Applicable Standard | Details |
|-----------------------------------------------------------------------------------|--------|---------------------------------------------------------------------------------------|------------------------------------|----------------------------------|
|  | CSA | Class I, Div 2 Groups A, B, C & D; T4 Class 1, Zone 2, AEx nA II T4 Ex nA II T4 | UL & CSA Standards | Certificate No. 06.CSA150464 |
|  | ATEX | II 3 G Ex nA II T4 | EN60079-0:2006 EN 60079-15:2005 | KEMA 06ATEX0251 X |
|  | CE | EMC Directive 2014/30/EU | EN:61326-1:2013 | EMC |
| | | RoHS Directive 2011/65/EU | | RoHS |
| | | Pressure Equipment Directive 2014/68/EU | | Sound Engineering Practice (SEP) |

Hazardous Location Classification

The modules shall be installed in a suitable enclosure providing a degree of protection of at least IP54 according to EN 60529, taking into account the environmental conditions under which the equipment will be used. Provisions shall be made to prevent the rated voltage from being exceeded by transient disturbances of more than 40%.

| Code Description | Code Option | Option Description | | | |
|--------------------------------|-------------|-----------------------------------------------------------------------------|--------------------|-------------------|-------------------|
| I. Base Model Code | 4850 | Flow Controller, Body 0 (50 sccm - 40 slpm) | | | |
| | 4860 | Flow Meter, Body 0 (50 sccm - 40 slpm) | | | |
| II. Digital I/O Communications | A | RS-232 + Analog, Select applicable analog I/O | | | |
| III. Model Revision Level | B | Revision | | | |
| IV. Analog I/O, Input / Output | B | 0-5 Vdc / 0-5 Vdc | | | |
| | C | 4-20 mA / 4-20 mA | | | |
| | D | 0-5 Vdc / 4-20 mA | | | |
| | E | 4-20 mA / 0-5 Vdc | | | |
| | 0 | None | | | |
| V. Power Supply | 1 | 15 Vdc | | | |
| | 2 | 24 Vdc | | | |
| VI. Mechanical Connections | 1A | 9/16" -18unf straight thread | | | |
| | B1 | 1/4" tube compression w/filter | | | |
| | C1 | 1/8" tube compression w/filter | | | |
| | D1 | 3/8" tube compression w/filter | | | |
| | E1 | 1/4" VCR w/filter | | | |
| | F1 | 1/4" VCO w/filter | | | |
| | G1 | 1/4" NPT-F w/filter | | | |
| | H1 | 6mm tube compression w/filter | | | |
| | J1 | 10mm tube compression w/filter | | | |
| | S1 | Downport, no O-ring cavity | | | |
| | T1 | 1/4" RC (BSPT) w/filter | | | |
| | X1 | Downport, with O-ring cavity | | | |
| | Y1 | 1/4" tube w/filter (5850TR replace) | | | |
| VII. Body | | Body | O-Ring Seal | Seat | Valve Type |
| | A | 316SS | Viton | None (Meter Only) | None (Meter Only) |
| | B | 316SS | Viton | Viton | Normally Closed |
| VIII. Area Classification | 1 | Standard Location (Safe Area) | | | |
| | 2 | ATEX Zone 2 | | | |
| | 4 | CSA Div 2/Zone 2 (Recognized) | | | |
| IX. Valve Orifice Size | A | No Orifice (Meter Only) | | | |
| | B | 0.001 inch / 0.03mm | | | |
| | C | 0.002 inch / 0.05mm | | | |
| | D | 0.003 inch / 0.08mm | | | |
| | E | 0.005 inch / 0.125mm | | | |
| | F | 0.008 inch / 0.2mm | | | |
| | G | 0.012 inch / 0.315mm | | | |
| | H | 0.020 inch / 0.5mm | | | |
| | J | 0.031 inch / 0.8mm | | | |
| | K | 0.049 inch / 1.25mm only available with power supply option code=2 (24 Vdc) | | | |

| Code Description | Code Option | Option Description | | |
|------------------------------|-------------|---------------------------------------------------------------------------------------------|-------------------------------------------------------------------|-----------------------------------------------|
| X. Mass Flow Restrictor Type | | Type or Restrictor | Restrictor Range (sccm N₂ Equivalent @ 0°C ref) | |
| | A | No Restrictor | N/A | N/A |
| | C | Plug | 0 | 180 |
| | K | K | 160.4 | 228.53 |
| | M | M | 218.4 | 310.6 |
| | N | N | 265.7 | 377.7 |
| | P | P | 332 | 471.6 |
| | Q | Q | 424.8 | 603 |
| | R | R | 554.8 | 787 |
| | S | S | 736.7 | 1044.6 |
| | T | T | 991.4 | 1405 |
| | U | U | 1348 | 1910 |
| | V | V | 1847 | 2617 |
| | W | W | 2546 | 3607 |
| | X | X | 3524 | 4992 |
| | Y | Y | 4894 | 6932 |
| | 1 | 1 | 6811 | 9647 |
| 2 | 2 | 9496 | 13,453 | |
| 3 | 3 | 13,250 | 18,773 | |
| 4 | 4 | 18,520 | 30,143 | |
| 5 | 5 | 30,100 | 50,143 | |
| XI. Calibration | | Calibration Condition | Accuracy | Traceability |
| | A | None-Uncalibrated | N/A | N/A |
| | B | Single Gas | ±3.0% of F.S. | None |
| | C | Single Gas | ±1.0% of F.S. | None |
| | E | Single Gas | ±1.0% of F.S. | ICC - International Calibration Certification |
| XII. Accessories | 0 | None | | |
| | 1 | LOI with Power Adapter | | |
| | 2 | LOI without Power Adapter | | |
| XIII. Certificates | 0 | None | | |
| | 9 | Multiple Certs. Describe required certs in notes. Add all applicable changes to list price. | | |
| | A | Declaration of Compliance 2.1 (Certificate of Conformance) | | |
| | B | Declaration of Compliance 2.1 Leak Test | | |
| | C | Declaration of Compliance 2.1 Pressure Test | | |
| | D | Declaration of Compliance 2.1 Oxygen Service | | |
| | E | Declaration of Compliance 2.1 Materials | | |
| XIV. OEM Code | A | Standard Brooks Label | | |

Sample Model Code

| I | II | III | IV | V | VI | VII | VIII | IX | X | XI | XII | XIII | XIV |
|------|----|-----|----|---|----|-----|------|----|---|----|-----|------|-----|
| 4850 | A | B | B | 1 | 1A | A | 2 | D | K | E | 2 | 9 | A |

Brooks is committed to assuring all of our customers receive the optimal solution for their application, along with outstanding service and support to back it up. We operate first class repair facilities located around the world to provide rapid response and support. Each location utilizes primary standard calibration equipment to ensure accuracy and reliability for repairs and recalibration and is certified by our local Weights and Measures Authorities and traceable to the relevant International Standards.

Visit www.BrooksInstrument.com to locate the service location nearest to you.

START-UP SERVICE AND IN-SITU CALIBRATION

Brooks Instrument can provide start-up service prior to operation when required. For some process applications, where ISO-9001 Quality Certification is important, it is mandatory to verify and/or (re)calibrate the products periodically. In many cases this service can be provided under in-situ conditions, and the results will be traceable to the relevant international quality standards.

SEMINARS AND TRAINING

Brooks Instrument can provide customer seminars and dedicated training to engineers, end users, and maintenance persons. Please contact your nearest sales representative for more details. Due to Brooks Instrument's commitment to continuous improvement of our products, all specifications are subject to change without notice.



TRADEMARKS

Brooks Brooks Instrument, LLC

All other trademarks are the property of their respective owners.

Data-Sheet-4800-EN/2024-12

Global Headquarters

Brooks Instrument
407 West Vine Street
Hatfield, PA
19440-0903 USA

Toll-Free (USA): 888-554-FLOW
T: 215-362-3500

BrooksAM@BrooksInstrument.com

A list of all Brooks Instrument locations and contact details can be found at www.BrooksInstrument.com

© Copyright 2024 Brooks Instrument, LLC All rights reserved. Printed in U.S.A.